
Mirpeptide
Laboratory2635
Parkmont Ln
Olympia, Wa

Certificate of Analysis

HCG 5000 IU

Report To:
Mirpeptide

Compound: HCG
Amount: 5000 IU
Laboratory ID: V260522-2 001
Lot Number: 260417HC50003
Date Released: 6/11/2026

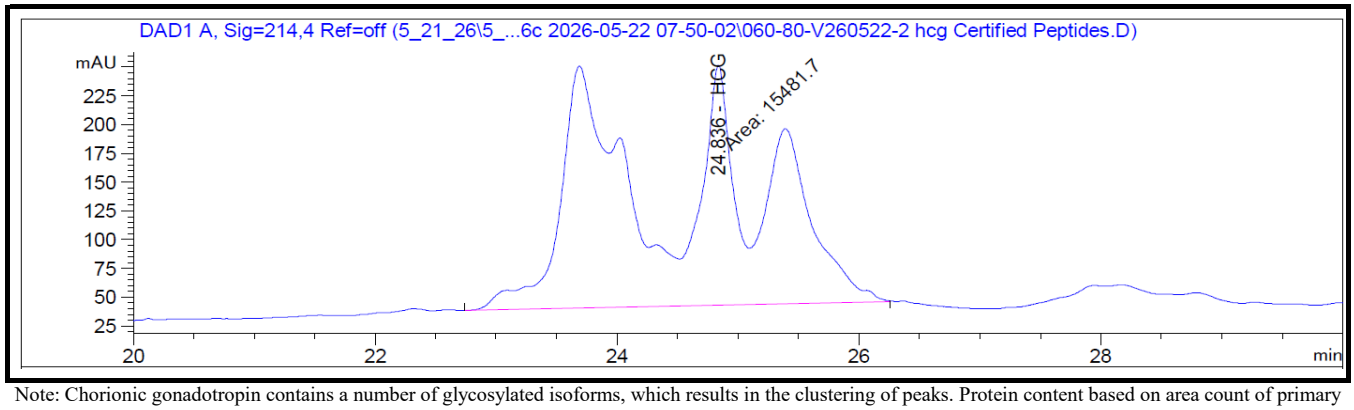

Note: Chorionic gonadotropin contains a number of glycosylated isoforms, which results in the clustering of peaks. Protein content based on area count of primary isoforms in comparison to certified reference standard. Per USP-NF a bioassay is required to accurately determine IU, HPLC-UV-Vis can be used to estimate HCG protein content

Analysis	Method	Result
Chromatographic Identification	HPLC-UV/VIS	Matches Standard
Quantity	HPLC-UV/VIS	~4800 IU



ISO 17025:2017 ACCREDITED LABORATORY

Report By: Dustin Newman, Laboratory Director on 6/11/2026

Approved By: Tori Johnson, Operations Manager on 6/11/2026

For a list of accredited test items, please refer to A2LA Certificate No. 6377.01.01. The condition of the samples upon receipt met the requirements. The results in this report apply only to the tested portion of the samples. All analyses were conducted in accordance with the Mirpeptide Laboratory's quality management system. Neither the Mirpeptide Laboratory nor its staff observed or participated in the sample selection process; therefore, we cannot confirm the authenticity of the samples or their representativeness of the relevant lots/batches.

https://mirpeptide.com
Prismapept@gmail.com

Mirpeptide
Laboratory2635
Parkmont Ln
Olympia, Wa

Certificate of Analysis

HCG 5000 IU

Report To:
Mirpeptide

Compound: HCG
Amount: 5000 IU
Laboratory ID: V260522-2 001
Lot Number: 260417HC50003
Date Released: 6/11/2026

Analyte	Method	LOQ (ppm)	Result (ppm)
Arsenic (As)	ICP-MS	0.01	ND
Cadmium (Cd)	ICP-MS	0.01	ND
Lead (Pb)	ICP-MS	0.01	ND
Mercury (Hg)	ICP-MS	0.005	ND

Run ID: 260531

Analysis	Method	Result
Endotoxins	LAL	Pass - <5.00 EU/mg*
Sterility	USP <71>	Pass - No Growth Detected

*Pass/Fail criteria based on the USP/FDA threshold of 5 EU/kg (350 EU total for a 70 kg adult)

Report By: Dustin Newman, Laboratory Director on 6/11/2026

Approved By: Tori Johnson, Operations Manager on 6/11/2026

ND: Non-Detect
LOD: Limit of Quantification

ISO 17025:2017 ACCREDITED LABORATORY

For a list of accredited test items, please refer to A2LA Certificate No. 6377.01.01. The condition of the samples upon receipt met the requirements. The results in this report apply only to the tested portion of the samples. All analyses were conducted in accordance with the Mirpeptide Laboratory's quality management system. Neither the Mirpeptide Laboratory nor its staff observed or participated in the sample selection process; therefore, we cannot confirm the authenticity of the samples or their representativeness of the relevant lots/batches.